




AUTOMATED AUDIOMETRY TESTING




GSi AMTAS

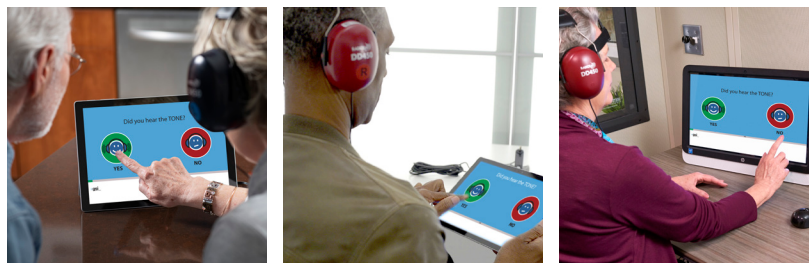

■ BY AUDIOLOGISTS, ■ FOR AUDIOLOGISTS

VALIDATED AND ACCURATE

GSI AMTAS™, or Automated Method for Testing Auditory Sensitivity, is a patient directed evaluation tool that uses patented test methods and accuracy algorithms to obtain diagnostic or screening audiometry. **With over 20 years of research and development**, the validity of GSI AMTAS has been proven through comprehensive studies.

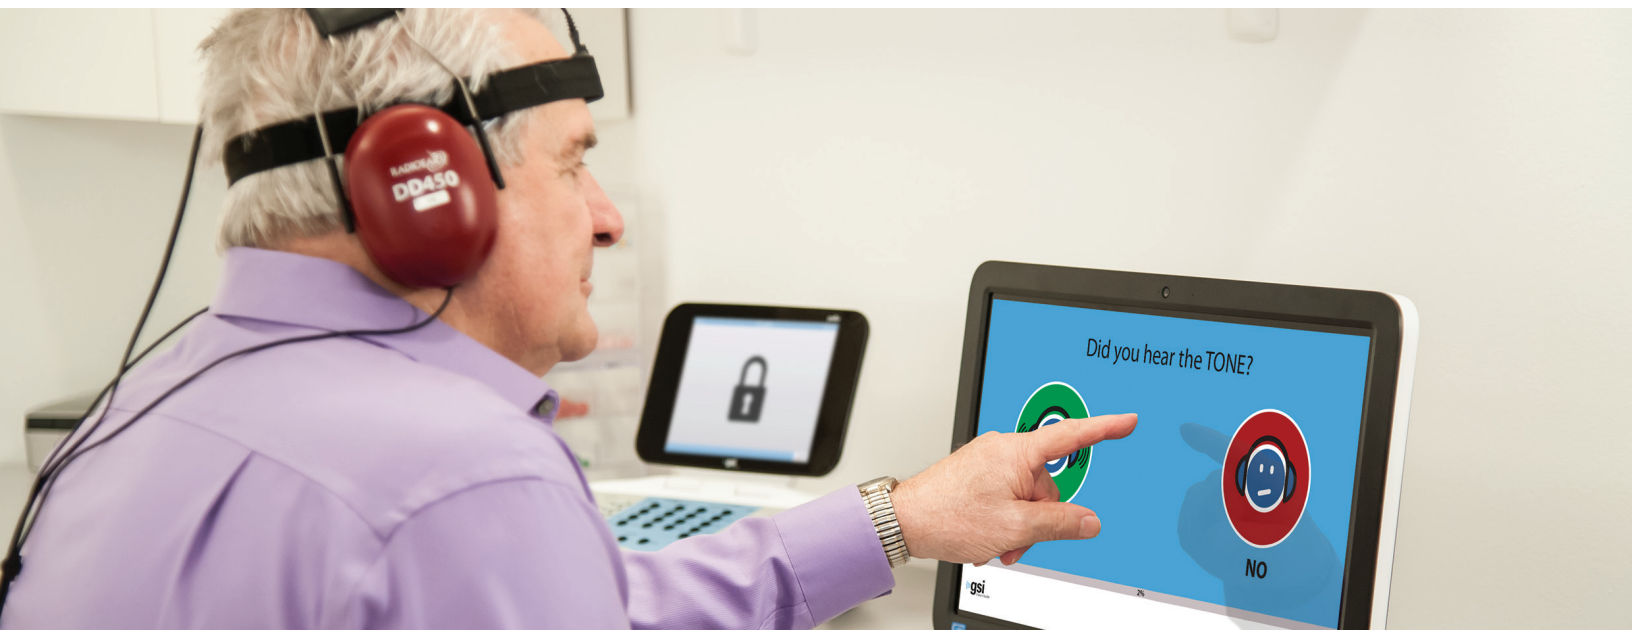

FOCUS ON PATIENT CARE

GSI AMTAS was created as a resource for clinicians to help manage their busy schedules and promote an efficient office environment. Most importantly, GSI AMTAS frees up the clinician, allowing more time to focus on patient care.

GSI AMTAS is available in two versions, GSI AMTAS Pro™ and GSI AMTAS Flex™, which give the hearing professional options to best fit specific clinical needs. With numerous comprehensive studies backed by years of research and development, GSI AMTAS is different from other automated audiometric tests. GSI AMTAS provides up to nine quality indicators, classification of audiometric findings, and two report formats.






3 KEY BENEFITS



WALK-IN PATIENTS

In a busy practice, GSI AMTAS helps the clinician manage more than one patient at a time. Basic diagnostic testing can be completed with one patient using GSI AMTAS while the clinician can tend to the needs of other patients.



APPOINTMENTS ARE STREAMLINED

When a patient returns for an annual evaluation, the clinician can get them started with GSI AMTAS while a clean and check of hearing aids is completed.



PATIENT COUNSELING


Quality indicators and the classification of audiometric findings give clinicians the tools required to determine the most appropriate next steps in testing and follow up.



GSI AMTAS PRO & GSI AMTAS FLEX

DIAGNOSTIC AUDIOMETRY

GSI AMTAS Pro offers diagnostic air conduction, bone conduction, and speech (SRT and WRS) testing with masking. This self-directed test typically takes about 15 minutes to complete and the report provides quality indicators to assist the clinician in determining the accuracy of the test. AMTAS Pro is operated through a computer connected to a compatible GSI Audiometer.

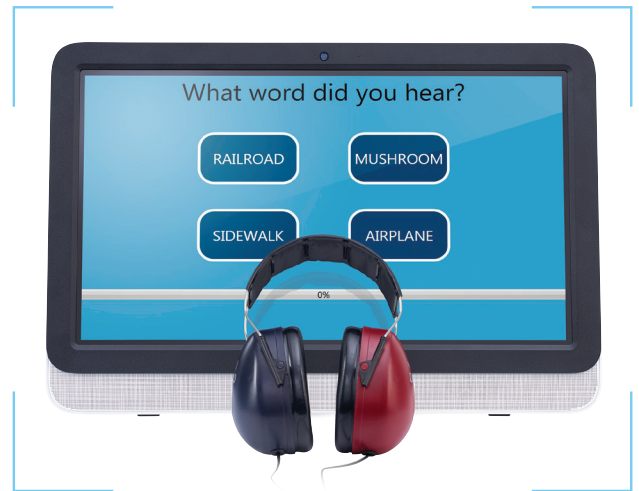

SCREENING AUDIOMETRY

GSI AMTAS Flex is tablet-based and does not require an audiometer. This version offers air conduction screening and threshold audiometry. The screening test is configurable and displays a Pass or Refer at the completion of the test. The threshold test provides six quality indicators and the AMCLASS audiogram classification.

REPORTING

GSI AMTAS generates two report formats. The Audiologist Report includes the audiogram and the quality assessment table with the quality indicators, AMCLASS™ audiogram classification, and a comprehensive speech audiometry table. The Patient Report includes an easy to understand description of hearing loss and the audiometric findings.

AUDIOGRAM CLASSIFICATION

GSI AMTAS includes a patented method of classifying audiometric findings, called AMCLASS, which summarizes the audiogram based on configuration, site of lesion, and severity. This provides further insight to the clinician on how to proceed with counseling and follow up testing if needed.




REPORTING OPTIONS

GSi AMTAS PRO



GSi-AMTAS™ Hearing Report

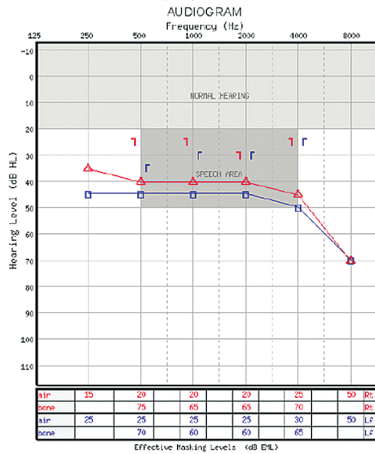


QUALITY ASSESSMENT (Air & Bone)	
Predicted Accuracy	GOOD
Quality Indicators	Value File
Predicted Avg. Abs. Diff. (dB)	5.287 6
Flasher HIRE (s)	0.000 6
Time per Trial (s)	2.698 6
False Alarm (s)	3.846 35
Avg. Test Retest Diff. (dB)	0.000 45
QC Fail (s)	0.000 6
ABR > 35	0.000 6
ABR < -10	0.000 6
LEGEND	Flasher HIRE
Masked Air	▲ 6
Masked Bone	■ 6

AMCLASS® Audiogram Classification			
Ear	Severity	Configuration	Site of Lesion
Right	MODERATE	Flat Hearing Loss	HEARD
Left	MODERATE	Flat Hearing Loss	HEARD
Symmetric			
Speech Recognition Report			
Ear	Pure Tone Avg. dB HL	SRT	Word Recognition Level (dB HL)
Right	40	45	75
Left	40	45	75

GSi AMTAS FLEX



GSi-AMTAS™ Hearing Report

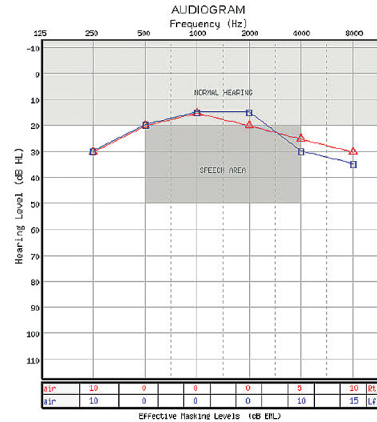

QUALITY ASSESSMENT (Air Only)	
Predicted Accuracy	GOOD
Quality Indicators	Value File
Predicted Avg. Abs. Diff. (dB)	2.077 25
Time per Trial (s)	4.768 30
False Alarm (s)	0.000 6
Avg. Test Retest Diff. (dB)	0.000 6
QC Fail (s)	0.000 6

LEGEND	Flasher HIRE
Masked Air	▲ 6

AMCLASS® Audiogram Classification			
Ear	Severity	Configuration	Site of Lesion
Right	MODERATE	Flat Hearing Loss	HEARD
Left	MODERATE	Flat Hearing Loss	HEARD
Symmetric			
PTA			
Ear	Pure Tone Avg. dB HL	SRT	Word Recognition Level (dB HL)
Right	40	45	75
Left	40	45	75





QUALITY INDICATORS



PREDICTED ACCURACY

Summary measure that categorizes the accuracy of the audiogram as Good, Fair, or Poor.



PREDICTED ABSOLUTE AVERAGE DIFFERENCE

The predicted difference between automated and manual thresholds based on research studies.



MASKER ALERTS*

The thresholds where masking may have been too high or too low.



TIME PER TRIAL

The average time it took the patients to respond to the stimulus.



FALSE ALARM RATES

The number of times the patient responded "yes" when no stimulus was presented, divided by the total number of times no stimulus was presented.



AVERAGE TEST-RETEST DIFFERENCE

The average difference between the initial 1000 Hz threshold and the second (retested) 1000 Hz threshold obtained for the right and left ears.



QUALITY CHECK FAIL RATE

The number of times the patient did not respond to stimulus above threshold, divided by number of measured thresholds.



NUMBER OF AIR/BONE GAP >35 DB*

The number of air/bone gaps that exceed 35 dB.



NUMBER OF AIR/BONE GAP <-10 DB*

The number of air/bone gaps that are less than -10 dB.

**Additional indicators only available on AMTAS Pro.*

■ WHAT YOU SHOULD EXPECT FROM OUR DEVICES


WORLD LEADER IN AUDIOMETRIC SOLUTIONS

GSI is a world leader in audiometric assessment instrumentation and carries a full line of audiometers, tympanometers, otoacoustic emissions (OAE), and auditory evoked potential instruments. From research facilities to school screenings, GSI instruments have been the equipment of choice for audiological assessments throughout the world for over 75 years.

DESIGNED SMART, BUILT STRONG

Our motto is Designed Smart, Built Strong. GSI devices are Designed Smart with the audiologist in mind, providing superior ergonomic design and navigation with one button, one function accessibility. Built Strong, our devices can take on the most routine to complex testing scenarios in any environment.

Quality, Reliable, and User-Friendly are the three core attributes that are the backbone of the GSI brand. These attributes are what you should expect from any GSI product.

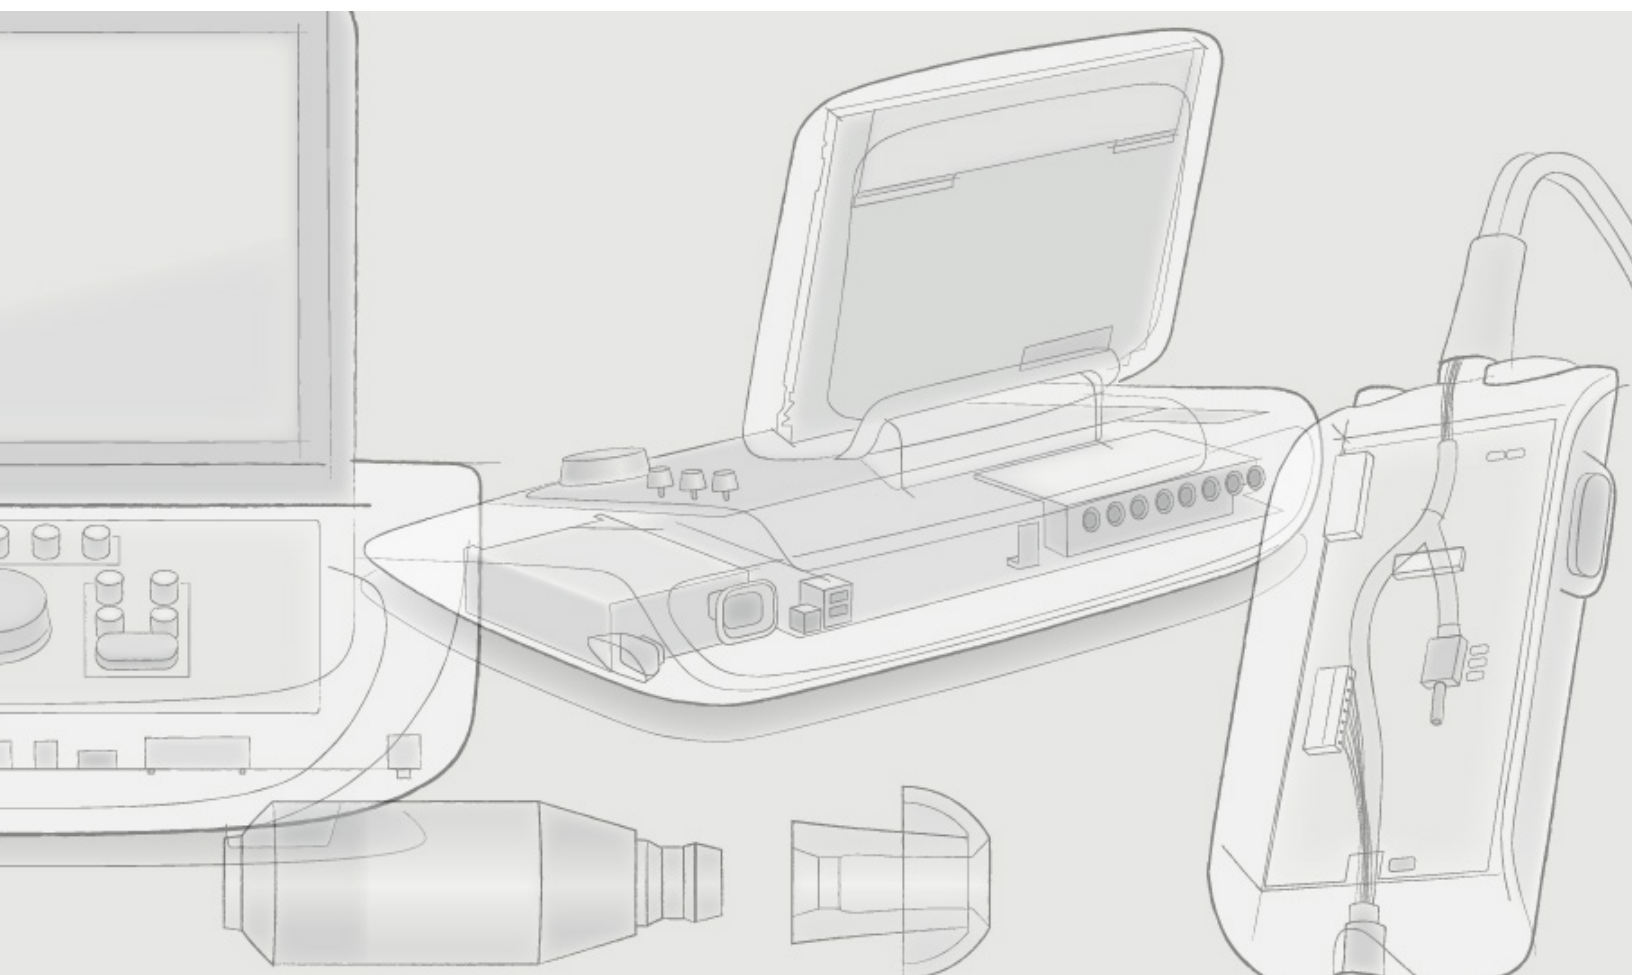

■ GSI AMTAS

TECHNICAL SPECIFICATIONS

- | | |
|---|--|
| <ul style="list-style-type: none"> • Air Conduction Diagnostic Frequencies: 250, 500, 750, 1000, 1500, 2000, 3000, 4000, 6000, 8000 Hz • Bone Conduction Diagnostic Frequencies: 500, 1000, 2000, 4000 Hz • Air Diagnostic Level Range: -20 to 100 dB HL • Bone Diagnostic Level Range: -20 to 75 dB HL (frequency dependent) | <ul style="list-style-type: none"> • Masking: Narrow band noise, speech noise • Air Conduction Screening Frequencies: 500, 1000, 2000, 4000 Hz • Air Conduction Screening Level: 20 or 25 dB HL • Speech Testing: Speech Recognition Threshold (SRT), Word Recognition Score (WRS) |
|---|--|

	GSI AMTAS FLEX	GSI AMTAS PRO
Air Conduction Diagnostic	✓	✓
Air Conduction Screening	✓	✓
Masking	✓	✓
Bone Conduction Diagnostic		✓
Speech SRT		✓
Speech WRS		✓
Connect to Audiometer		✓
VA Quasar Integration		✓
dB HL Range	10 to 80	-20 to 100
Quality Indicators	✓	✓
Audiogram Classification	Limited	Comprehensive